



Standard Test Method for Pyrometric Cone Equivalent (PCE) of Fireclay and High Alumina Refractory Materials¹

This standard is issued under the fixed designation C 24; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reappraisal. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reappraisal.

This standard has been approved for use by agencies of the Department of Defense.

1. Scope

1.1 This test method covers the determination of the Pyrometric Cone Equivalent (PCE) of fire clay, fireclay brick, high alumina brick, and silica fire clay refractory mortar by comparison of test cones with standard pyrometric cones under the conditions prescribed in this test method.

1.2 *Units*—The values stated in inch-pound units are to be regarded as standard. The values given in parentheses are mathematical conversions to SI units that are provided for information only and are not considered standard.

1.2.1 *Exceptions*—Certain weights are in SI units with inch-pound in parenthesis. Also, certain figures have SI units without parenthesis. These SI units are to be regarded as standard.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 *ASTM Standards*:²

C 71 Terminology Relating to Refractories

E 11 Specification for Wire Cloth and Sieves for Testing Purposes

E 220 Test Method for Calibration of Thermocouples By Comparison Techniques

E 691 Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method

3. Terminology

3.1 *Definitions*—For definitions of terms used in this test method, see Terminology **C 71**.

¹ This test method is under the jurisdiction of ASTM Committee **C08** on Refractories and is the direct responsibility of Subcommittee **C08.02** on Thermal Properties.

Current edition approved March 1, 2009. Published April 2009. Originally approved in 1919. Last previous edition approved in 2006 as C 24 – 01 (2006).

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

4. Summary of Test Method

4.1 This test method consists of preparing a test cone from a refractory material and comparing its deformation end point to that of a standard pyrometric cone. The resultant PCE value is a measure of the refractoriness of the material.

4.2 Temperature equivalent tables for the standard cones have been determined by the National Institute of Standards and Technology when subjected to both slow and rapid heating rates.

5. Significance and Use

5.1 The deformation and end point of a cone corresponds to a certain heat-work condition due to the effects of time, temperature, and atmosphere.

5.2 The precision of this test method is subject to many variables that are difficult to control. Therefore, an experienced operator may be necessary where PCE values are being utilized for specification purposes.

5.3 PCE values are used to classify fireclay and high alumina refractories.

5.4 This is an effective method of identifying fireclay variations, mining control, and developing raw material specifications.

5.5 Although not recommended, this test method is sometimes applied to materials other than fireclay and high alumina. Such practice should be limited to in-house laboratories and never be used for specification purposes.

6. Procedure

6.1 *Preparation of Sample*:

6.1.1 *Clay or Brick*—Crush the entire sample of fire clay or fireclay brick, in case the amount is small, by means of rolls or a jaw crusher to produce a particle size not larger than ¼ in. (6 mm). If the amount is large, treat a representative sample obtained by approved methods. Then mix the sample thoroughly and reduce the amount to about 250 g (0.5 lb) by quartering (see **Note 1**). Then grind this portion in an agate, porcelain, or hard steel mortar and reduce the amount again by quartering. The final size of the sample shall be 50 g and the

fineness capable of passing an ASTM No. 70 (212- μ m) sieve³ (equivalent to a 65-mesh Tyler Standard Series). In order to avoid excessive reduction to fines, remove them frequently during the process of reduction by throwing the sample on the sieve and continuing the grinding of the coarser particles until all the sample passes through the sieve (see **Note 2**). Take precautions to prevent contamination of the sample by steel particles from the sampling equipment during crushing or grinding.

NOTE 1—Take care during the crushing and grinding of the sample to prevent the introduction of magnetic material.

NOTE 2—The requirement to grind the coarser particles is particularly important for highly siliceous products; excessively fine grinding may reduce their PCE by as much as two cones.

6.1.2 *Silica Fire Clay* (see 3.1)—In the case of silica fire clay, test the sample obtained by approved methods as received without grinding or other treatment.

6.2 *Preparation of Test Cones:*

6.2.1 After preparing samples of unfired clays (**Note 3**), or of mixes containing appreciable proportions of raw clay, in accordance with 6.1.1, heat them in an oxidizing atmosphere in the temperature range from 1700 to 1800°F (925 to 980°C) for not less than 30 min.

NOTE 3—Some unfired clays bloat when they are formed into cones and are carried through the high-temperature heat treatment prescribed in 5.4.1 without preliminary calcining. The substances that cause bloating can, in most cases, be expelled by heating the clay samples before testing.


6.2.2 The clay sample may be given the heat treatment prescribed in 6.2.1 after it has been formed into a cone (see 6.2.3), but this procedure has been found not as effective as the treatment of the powdered material. If cones so prepared bloat during the PCE test, heat a portion of the original sample in its powdered condition as prescribed in 6.2.1 and then retest it.

6.2.3 Thoroughly mix the dried sample, and after the addition of sufficient dextrine, glue, gum tragacanth, or other alkali-free organic binder and water, form it in a metal mold into test cones in the shape of a truncated trigonal pyramid with its base at a small angle to the trigonal axis, and in accordance with dimensions shown in **Fig. 1**. In forming the test cone use the mold shown in **Fig. 2**.

6.3 *Mounting:*

6.3.1 Mount both the test cones and the Standard Pyrometric Cones on plaques of refractory material that have a composition that will not affect the fusibility of the cones (see **Note 4**). Mount both test and PCE cones with the base embedded so that the length of the sloping face of the cone above the plaque shall be $1\frac{5}{16}$ in. (24 mm) and the face of the cone (about which bending takes place) shall be inclined at an angle of 82° with the horizontal. Arrange the test cones with respect to the PCE cones as shown in **Fig. 3**, that is, alternate the test cones with the PCE cones in so far as is practical (see **Note 5**). The plaque may be any convenient size and shape and may be biscuited before using, if desired.

NOTE 4—A satisfactory cone plaque mix consists of 85 % fused alumina and 15 % plastic refractory clay. For tests that will not go above

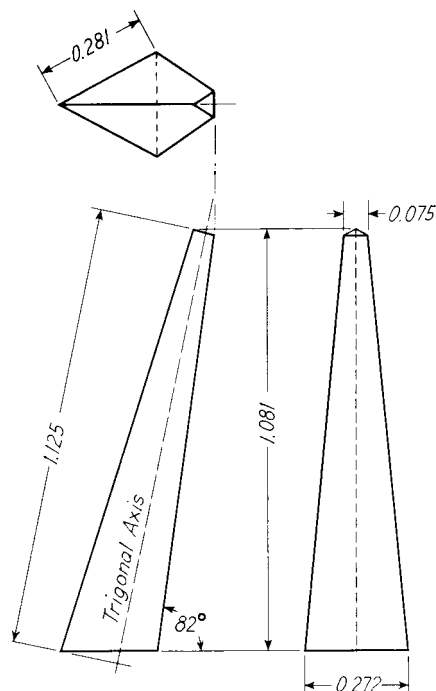

NOTE 1—Dimensions are in inches.

SI Equivalents

in.	mm
0.075	1.90
0.272	6.91
0.281	7.14
1.081	27.46
1.125	28.58

FIG. 1 Standard Pyrometric Test Cone

Cone 34, the plastic refractory clay may be increased to 25 % and the alumina may be replaced with brick grog containing over 70 % alumina. The alumina or grog should be ground to pass an ASTM No. 60 (250- μ m) sieve (equivalent to a 60-mesh Tyler Standard Series), and the PCE of the refractory plastic clay should be not lower than Cone 32.

NOTE 5—The number of cones and their mounting facing inward as shown in **Fig. 3** is typical for gas-fired furnaces of relatively large dimensions and gases moving at high velocity. The practical bore of the muffle tubes in most electric furnaces does not permit cone pats of this size. The static atmosphere prevailing permits the cones being mounted to face outward, if so desired.

6.4 *Heating:*



6.4.1 Perform the heating in a suitable furnace, operating with an oxidizing atmosphere, at rates to conform to the following requirements (see **Note 6** and **Note 7**). It is advisable, but not mandatory that the furnace temperature be controlled with a calibrated⁴ thermocouple or radiation pyrometer connected to a program-controlled recorder.

6.4.1.1 For PCE tests expected to have an end point of PCE Cone 12 or above, but not exceeding Cone 26, heat at the rate prescribed in **Table 1**.

6.4.1.2 For PCE tests expected to have an end point above Cone 26, heat at the rate prescribed in **Table 2**.

³ Detailed requirements for this sieve are given in Specification **E 11**.

⁴ Test Method **E 220** specifies calibration procedures for thermocouples.

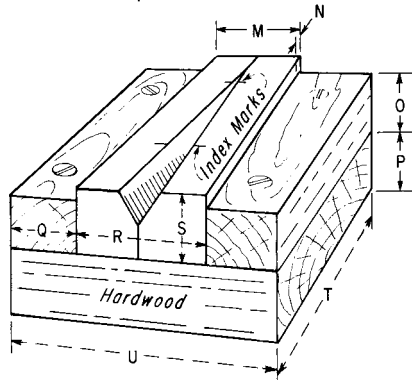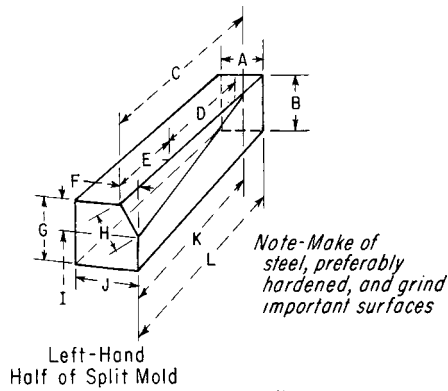

Note - Index marks show the length of the short side of the cone

Mold Assembly

Table of Dimensions

	in.	mm		in.	mm
A	0.50	12.7	K	2.500	63.50
B	0.75	19.0	L	2.75	69.8
C	2.510	63.75	M	1.00	25.4
D	1.084	27.53	N	0.12	3.0
E	1.015	25.78	O	0.62	15.7
F	0.229	5.82	P	0.75	19.0
G	0.75	19.0	Q	0.75	19.0
H	0.460	11.68	R	1.50	38.1
I	0.399	10.13	S	0.75	19.0
J	0.75	19.0	T	2.62	66.5

FIG. 2 Split Mold for ASTM Pyrometric Test Cone

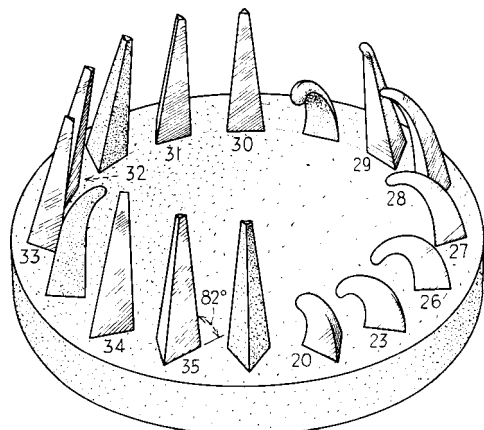


FIG. 3 Method of Mounting Test Cones and Appearance After Testing

TABLE 1 Heating Rates Up to Cone 26

Cold Test Furnace to Cone No.	Time interval, min	Cumulative Time, h:min
12	45	0:45
13	5	0:50
14	19	1:09
15	13	1:22
16	24	1:46
17	9	1:55
18	4	1:59
19	8	2:07
20	9	2:16
23	16	2:32
26	7	2:39

TABLE 2 Heating Rates Above Cone 26

Cold Test Furnace to Cone No.	Time Interval, min	Cumulative Time, h:min
20	45	0:45
23	16	1:01
26	7	1:08
27	7	1:15
28	3	1:18
29	5	1:23
30	3	1:26
31	7	1:33
31½	6	1:39
32	7	1:46
32½	3	1:49
33	7	1:56
34	9	2:05
35	9	2:14
36	7	2:21
37	7	2:28

NOTE 6—The heating rate through the cone series in both Table 1 and 2 is at 270°F (150°C)/h.

NOTE 7—Following a test run, the cone pat may be removed at 1830°F (1000°C) and a new pat may be put in without cooling the furnace to below red heat. The time interval to bring the furnace, using Table 1, up to Cone 12 shall be not less than 20 min, and using Table 2, the time interval up to Cone 20 shall be not less than 25 min.

6.4.2 The furnace atmosphere shall contain a minimum of 0.5 % oxygen with 0 % combustibles. Make provisions to prevent any external forces from being exerted on the cones or cone plaque, such as from flames or gases. Test the furnace at intervals to determine the uniformity of the distribution of the heat.

6.5 Pyrometric Cone Equivalent:

6.5.1 The softening of the cone will be indicated by the top bending over and the tip touching the plaque. Always report the bloating, squatting, or unequal fusion of small constituent particles. Report the Pyrometric Cone Equivalent (PCE) in terms of Standard Pyrometric Cones and the cone that most nearly corresponds in time of softening with the test cone. If the test cone softens later than one Standard Pyrometric Cone but earlier than the next Standard Pyrometric Cone and approximately midway between, report the PCE as Cone 33–34.

6.5.2 If the test cone starts bending at an early cone but is not down until a later cone, report this fact.

6.5.3 The temperatures corresponding to the end points of the Standard Pyrometric Cones are frequently of interest and are shown in **Appendix X1**.

7. Precision and Bias

7.1 *Precision*—No justifiable statement of precision is possible since the results of the tests are descriptive and do not produce a precise numeric value.

7.2 *Bias*—No justifiable statement on bias is possible since the true physical property values of refractories cannot be established by any acceptable reference material.

8. Keywords

8.1 PCE; pyrometric cone; pyrometric cone equivalent; refractories

APPENDIX

(Nonmandatory Information)

X1. TEMPERATURES CORRESPONDING TO STANDARD PYROMETRIC CONE END POINTS

TABLE X1.1 Temperature Equivalents for Pyrometric Cones Used in Refractory Testing

Cone No.	End Point, °F (°C)	Cone No.	End Point, °F (°C)
12	2439 (1337)	31	3061 (1683)
13	2460 (1349)	31½	3090 (1699)
14	2548 (1398)	32	3123 (1717)
15	2606 (1430)	32½	3135 (1724)
16	2716 (1491)	33	3169 (1743)
17	2754 (1512)	34	3205 (1763)
18	2772 (1522)	35	3245 (1785)
19	2806 (1541)	36	3279 (1804)
20	2847 (1564)	37	3308 (1820)
23	2921 (1605)	38	3335 (1835)
26	2950 (1621)	39	3389 (1865)
27	2984 (1640)	40	3425 (1885)
28	2995 (1646)	41	3578 (1970)
29	3018 (1659)	42	3659 (2015)
30	3029 (1665)		

X1.1 The approximate temperature equivalents corresponding to the end points of those Standard Pyrometric Cones that are used in connection with refractory testing are as shown in **Table X1.1**.

X1.2 Heating Rate:

X1.2.1 Cones 12 to 37, inclusive—270°F (150°C)/h.

X1.2.2 Cone 38—180°F (100°C)/h.

X1.2.3 Cones 39 to 42, inclusive—1080°F (600°C)/h.

X1.3 Standard Pyrometric Cones 28 and 30 are manufactured but are not used in the PCE test.

X1.4 Temperatures for Cones 12 to 37 were reported at the National Institute of Standards and Technology.⁵ Temperatures for Cones 38 to 42 were determined by C. O. Fairchild and M. F. Peters.⁶ These temperatures apply satisfactorily for all the conditions of this test method, but do not apply to the conditions of commercial firing of kilns and use of refractory materials.

X1.5 Temperature values were determined in degrees Celsius; Fahrenheit temperature values were calculated.

⁵ Beerman, H. P., *Journal of the American Ceramic Society*, Vol. 39, No. 2H, 1956, pp. 47–53.

⁶ Fairchild, C. O., and Peters, M. F., “Characteristics of Pyrometric Cones.” *Journal of the American Ceramic Society*, Vol. 9, No. 11, November 1976, p. 700.

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org).